MoblVac®

QUICK START TROUBLESHOOTING GUIDE

This unit is to be used by trained medical personnel only.
This guide is to be used as a quick reference for the operator.
Please refer to the operation manual supplied wih the unit for complete operating and usage instructions.

INVACARE

Yes, you can:

CONTINUOUS THERAPY MODE

1 Press “Power” button to begin. Green LED will illuminate and screen will power up.

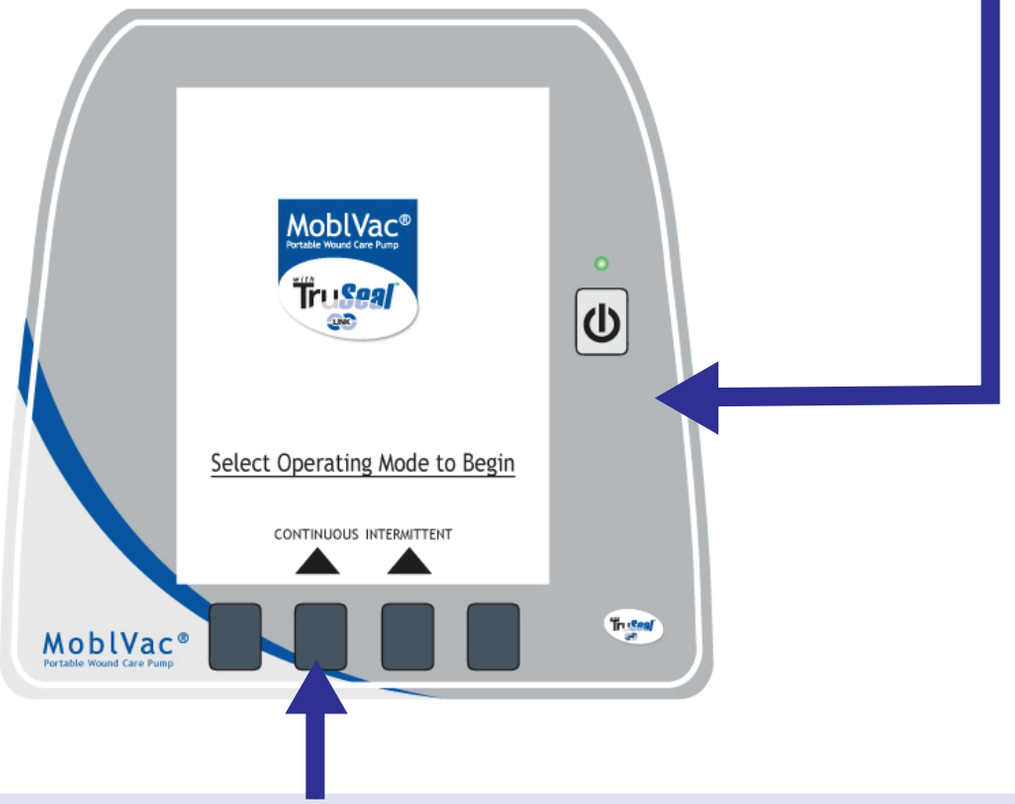

2 Press “Continuous” button. An audible noise will be heard as the pump begins to apply negative pressure.

Continue to next page

CONTINUOUS THERAPY MODE

3 Press “Increase” and set pressure to prescribed vacuum level.

INTERMITTENT THERAPY MODE

1 Press “Power” button to begin. Green LED will illuminate and screen will power-up. Thne press “Intermittent” button.

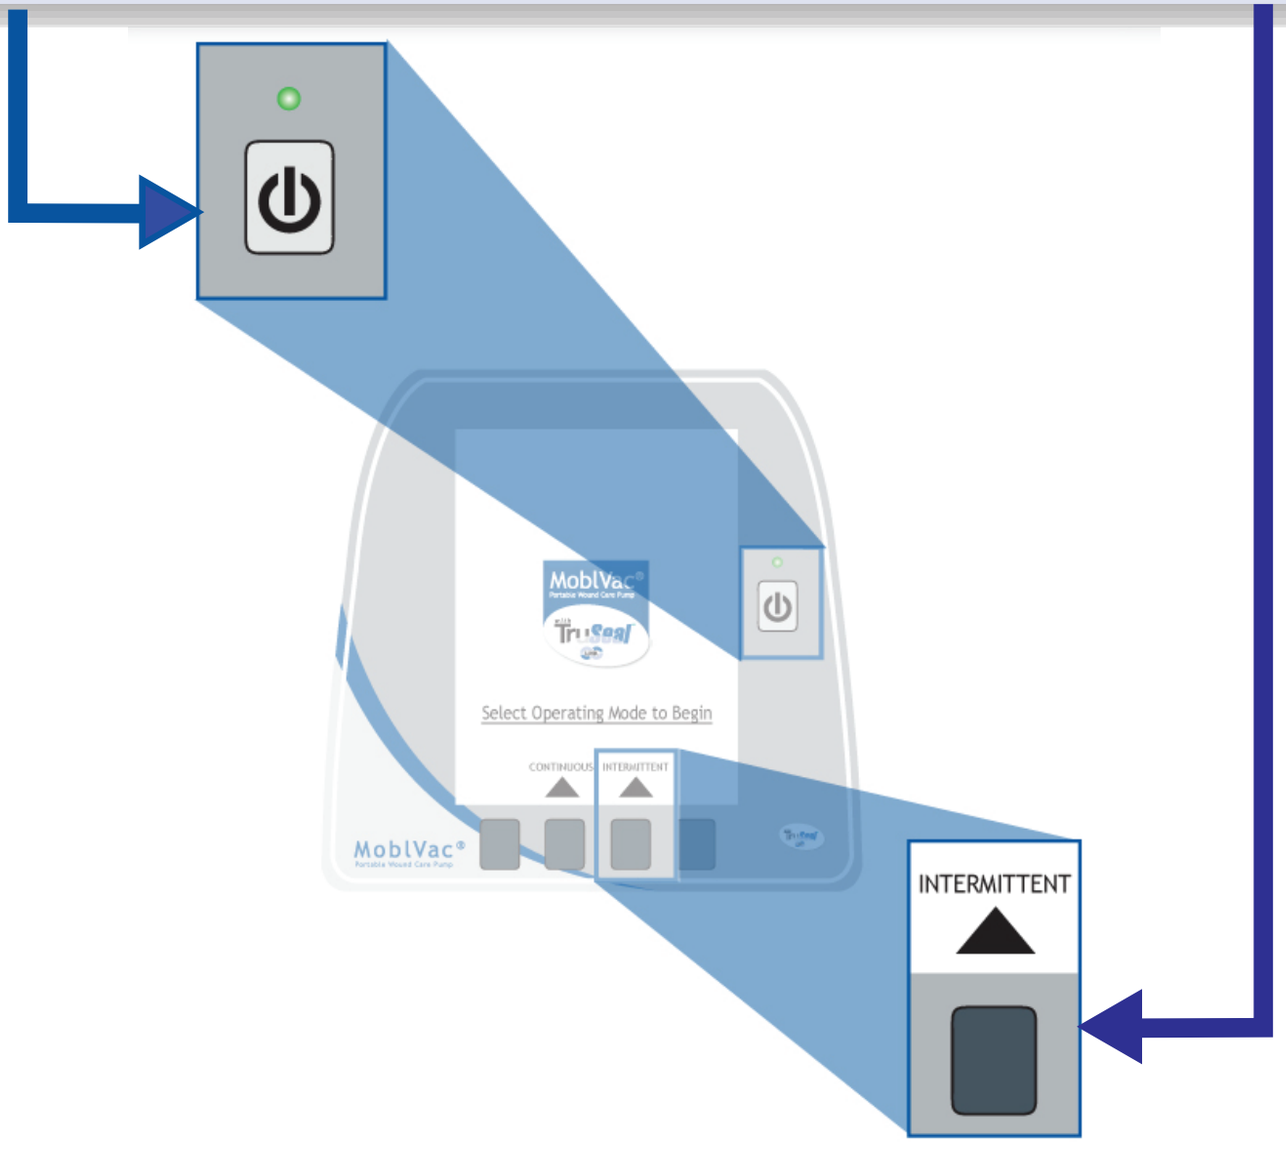

Continue to next page

INTERMITTENT THERAPY MODE

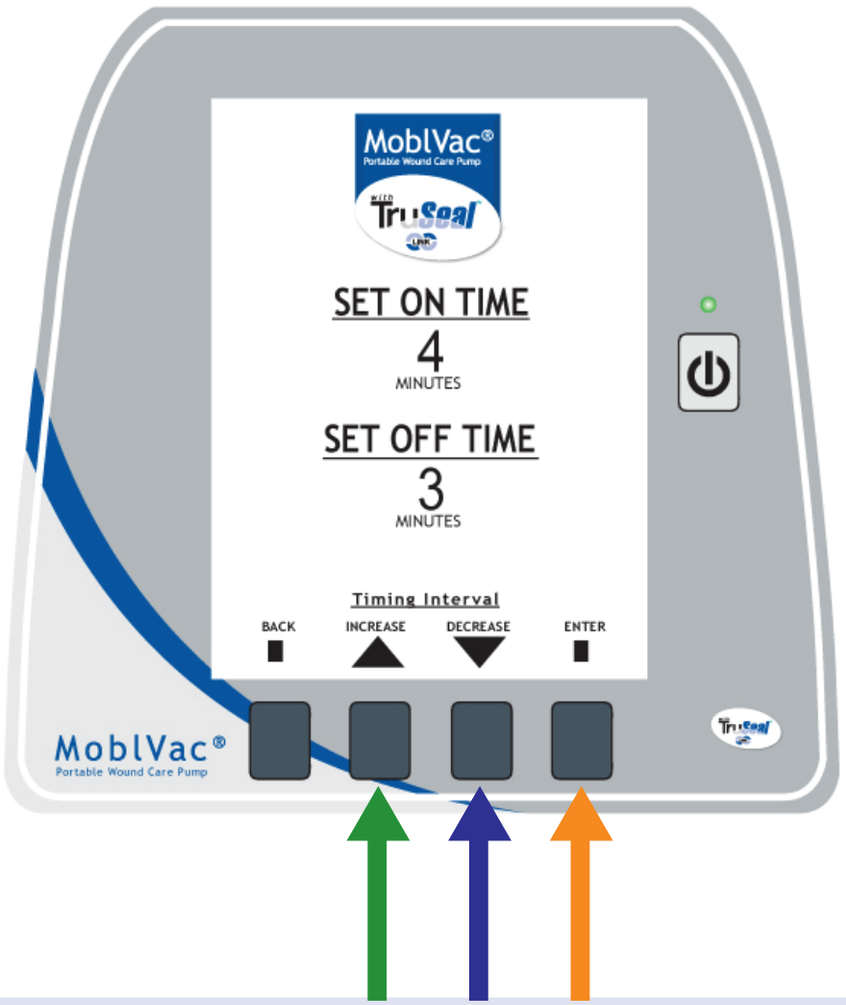

2 Press increase/decrease buttons to set the desired "On" timing. Press "Enter". Repeat for desired "Off" timing interval. Press "Enter" when done. Pump will begin to apply negative pressure.

Continue to next page

INTERMITTENT THERAPY MODE

3 Press “Increase” and set pressure to prescribed vacuum level.

OPTIONS

SLEEP MODE ILLUMINATION

Once the unit is set to the proper pressure and is operating normally, after approximately five minutes, the display will become black. This feature is intended to preserve battery life.

Green LED indicates unit is On

OR

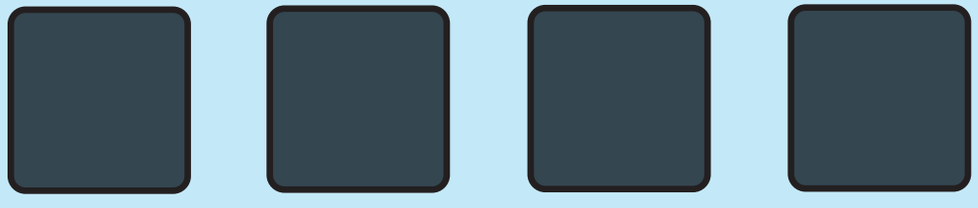

Press any of the bottom four buttons to illuminate display.

OPTIONS

NOTE: From the power up screen, press "Options" button to get "Options" screen.

TO TURN SLEEP MODE OFF

Press the "Sleep Off?" button. This will turn off the sleep mode and the screen will stay illuminated. Then press "Return" to go back to therapy operating mode. It is recommended to only use this feature when plugged into wall power as it will deplete the battery faster.

OPTIONS

TO ENGAGE LOCKOUT MODE

Press the “Lockout” button from the options menu to lock unit. This will disable the keypad and protect the settings from accidental button presses. The lockout icon will appear.

TO DISENGAGE LOCKOUT MODE

Press and hold the “Hold to Unlock” button and then simultaneously press the “Unlock” button that will appear on screen. This action will unlock the keypad.

SYMBOLS

SYMBOLS LEGEND

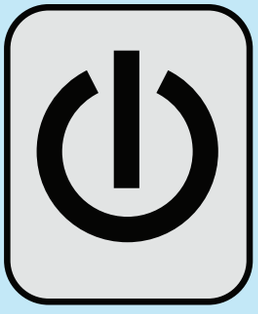

Power On/Off

Lockout Mode Active

Unit Connected to
Wall Power

SYMBOLS

SYMBOLS LEGEND

Battery Level Indicator

Green = Battery Charged*
Yellow = Battery Partially Charged*
Red = Battery Needs Charging*
Blank and Flashing = Battery nearly depleted
Plug in immediately.

*Assuming fully charged battery.

ALARMS

NOTE: To silence alarms for leak or canister, press the "Silence" button.

LEAK ALARM

If the system detects a leak, an audible alarm will sound, the pump will pulse frequently, and the display will flash this message:

LEAK ALARM

CORRECTIVE ACTION

- *Check dressing for "hissing" sound*
- *Seal edges with tape or additional film dressing*
- *Pinch paste around drain tube*
- *Ensure tubing is firmly connected to canister*
- *Press firmly on canister in a downward motion*

PAUSE REMINDER ALARM

If the unit is left in pause mode, the alarm will sound three times every five minutes to remind the user to restart the unit. To restart unit, press the "Run" button.

ALARMS

CANISTER ALARM

When the canister becomes full, negative pressure will cease, an audible alarm will sound, and the display will flash this message:

⚠ CANISTER ALARM ⚠

CORRECTIVE ACTION

- *Replace full canister and press "Run" to resume therapy*
- *Ensure unit is upright*

NOTE: You cannot silence this alarm until plugged into wall power.

PAUSE REMINDER ALARM

When the unit has approximately 10 minutes of battery operation remaining, an audible alarm will sound.

CORRECTIVE ACTION

- *Plug unit into wall power*

RE-ORDER PART NUMBERS

MoblVac® Wound Care Pump:
769600 MoblVac® Portable Wound Care Pump

Dressing Kits
Tri-Fold packaging with instructions for use:
769812 TruSeal™ Link Woundcare Kit (Value)
769813 TruSeal™ Link Woundcare Kit (Economy)
769814 TruSeal™ Link Woundcare Kit (Medium Channel)
769815 TruSeal™ Link Woundcare Kit (Small Round)
769816 TruSeal™ Link Woundcare Kit (X-Large Round)
769804 TruSeal™ Link Seal Kit

MoblVac® Accessories:
769703 Collection Canister with Solidifier
769703-NS Collection Canister without Solidifier
769605 Replacement Power Supply
769700 MoblVac® Premium Transport Bag
769606 Pole Clamp

⚠ WARNING

Monitor patient for excessive bleeding, which may result in serious injury or death.
If sudden or increased bleeding is observed, immediately stop therapy and seek medical attention.

Do not use this or any electrical device in an explosive or flammable environment or in the presence of flammable anesthetics.

Read, understand and follow the operation manual, including the clinical considerations/guidelines section for safe use. The user manual can be found at: www.MoblVacNPWT.com.

CONTACT US

Clinical/Technical Hotline
866.985.NPWT (6798)

www.MoblvacNPWT.com info_icc@invacare.com

Invacare Continuing Care, Inc.

USA
One Invacare Way
Elyria, Ohio USA
44036-2125

© 2011 Invacare Continuing Care Inc. All rights reserved. Republication, duplication or modification in whole or in part is prohibited without prior written permission from Invacare. Trademarks are identified by ™ and ® . All trademarks are owned by or licensed to Invacare Corporation or its subsidiaries unless otherwise noted.
Manufactured by Ohio Medical Corporation.

INVACARE

Yes, you can:

P/N 1176102 Rev A - 12/11